

Cleaning and Disinfection in Your Veterinary Clinic

How To Disinfect With Fuzion® In Vet Clinics



Kills bacteria, viruses, and fungi in 1 min, including canine parvovirus

Clorox Healthcare®
Fuzion® Cleaner Disinfectant
32 fl. oz. spray bottle



1. Put on PPE. Remove gross visible soil such as feces and bodily fluids prior to disinfecting.
2. If trigger is in locked position, squeeze the red tab under the nozzle and push downwards to unlock.
3. SPRAY 6" -8" from the surface until the surface is completely wet.
4. To **DISINFECT**, let stand for **1 MINUTE**. Then **WIPE** or **RINSE**. Allow to air dry.


Cleaning and Disinfecting Each Room

Use Clorox Healthcare® Fuzion® Cleaner Disinfectant


Follow these steps for effective cleaning




Exam rooms

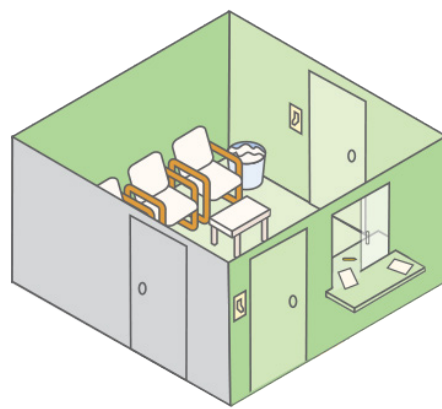

Waiting rooms

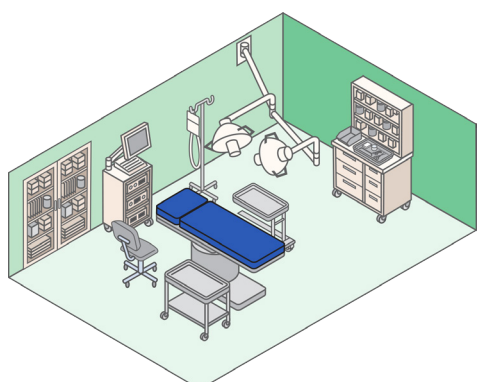

Procedural rooms

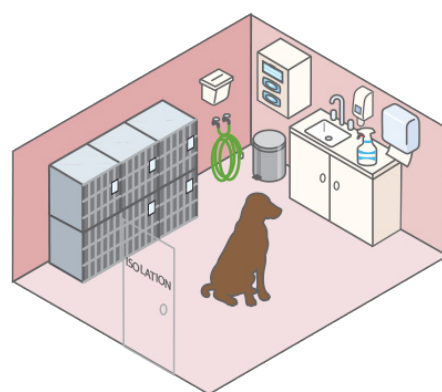

Isolation areas




PREPARE

Gather supplies, perform hand hygiene. Put on PPE.



INSPECT

Inspect the surface to see if there is any gross soil or foreign material.



REMOVE

Remove gross visible soil such as feces and bodily fluids before disinfecting.



APPLY

Apply the product to cover the surface.



WAIT

Ensure the surface remains wet for the 1 minute contact time.



WIPE AND DRY

Wipe surface with a microfiber cloth. Use clean cloths regularly.



POLISH

To protect surfaces, remove any excess residue with a clean, dry or damp cloth.